



CarePort Referral Form

Client Information:

Title: Full Name:

Address:

No: Street:

Suburb: Postcode:

Email: Phone:

DOB: Female: Male:

Funding Party:

Funding Party Contact Details:

Does the client have a NDIS Package? Y N NDIS Ref. No.

Is the package plan managed? Y N NDIS Plan Dates:

Plan Manager's Details:

Plan Manager's Email:

Source of Referral (E.G OT's Details)

Name:

Phone:

Email:

Organisation:

Client Contacts / Carer Information

Name:

Phone:

Email:

Is this contact/carer the person to liaise with?

Relationship to client:

CarePort Checklist:

This checklist will assist in identifying if a CarePort Unit is suitable for the person, and if the environment is suitable.

Has a **home visit** been conducted by the treating occupational therapist? Yes No

Proposed CarePort location:

Flooring Description:

Note – Cannot be installed on carpet.


Position of ORG, Garden Tap & Power point:

PLEASE PROVIDE A PHOTOGRAPHS OF THE PLANNED LOCATION AND POINTS ABOVE.

ARE THERE STEPS TO CAREPORT LOCATION? YES / NO, IF YES HOW MANY? _____

User Requirements:


- Shower Only Standard Model – 1010mm W x 1030 mm L Supply: Hot Water Unit
 Toilet Only Longer Model – 895mm W x 1215 mm L
 Shower and Toilet 120Plus – 1010mm x 1210mm L

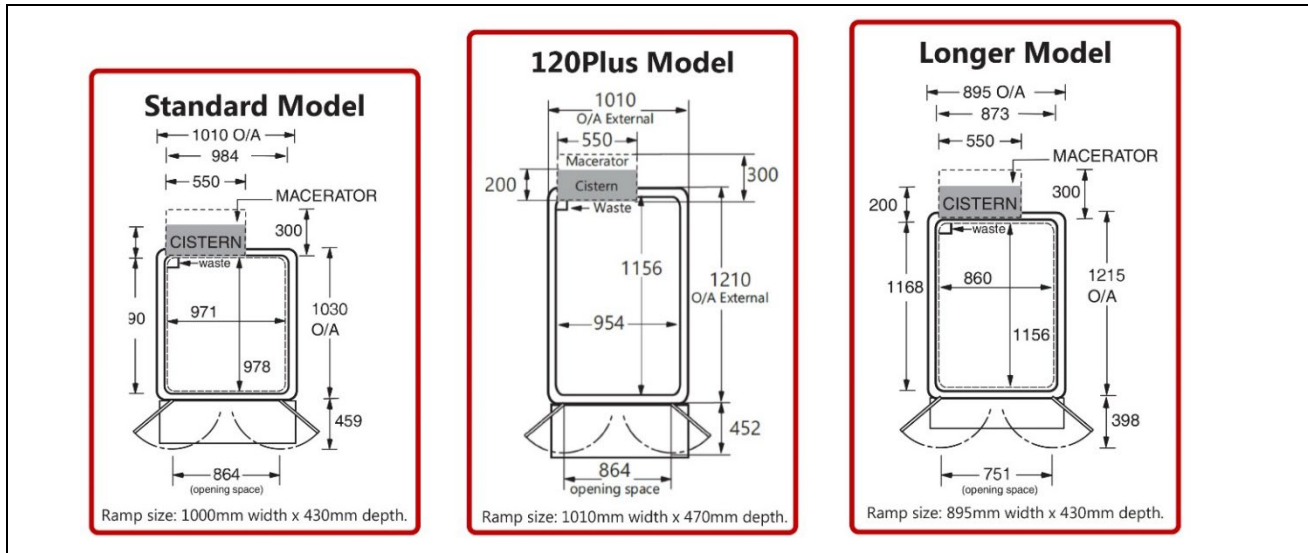

Internal Measurements for Commode Chairs

There is a pump in the back left cover (whilst looking at toilet). This may hinder the large Wheeled Commode Chairs. Measurements will need to be taken by OT to determine if commode will fit.

From left wall, the pump is 195mm Wide, 95mm to edge of pan. On the right side of the toilet pan there is 290mm to side wall.

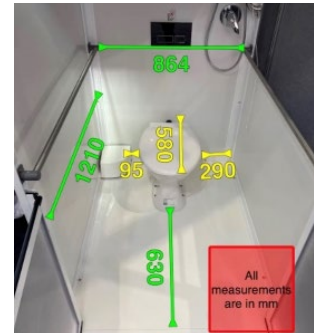

Purpose of CarePort:

- To facilitate discharge whilst waiting for bathroom modifications
 To facilitate discharge to a home with a bathroom that cannot be modified for the person's long-term requirements
 To facilitate discharge to a rental property

Anticipated length of need:

- 4 weeks 8 weeks 12 weeks 16 weeks

How did you hear about us?

Email referral form along with diagrams, photos and other necessary documents to enquiries@vipaccess.net.au to obtain a quote.

Please check our CarePort Video on this link <https://www.vipaccess.net.au/careport/>

Note - Careport Unit & Ramp can take a maximum of 200kg Safe Working Load and Grab Rails are for a maximum 80kg assistance only and not weight bearing.